



**LABORATORY FOR TESTING OF MACHINERY,  
EQUIPMENT AND DEVICES**  
**CENTER FOR TESTING AND EUROPEAN CERTIFICATION LTD**

2, Industrialna Str., Stara Zagora, Bulgaria,  
Tel.: +359 42 620 368 Fax: +359 42 602 377 ctec@ctec-sz.com

## TEST REPORT

Nº 2emc-i-14-906/ 20.06.2014

**OBJECT TO BE TESTED:** Luminaire „VIKIOM“ 4x14W/T5 with cat. Nº 9VOM414  
Representative sample from fixtures group „VIKI“ with cat. Nº: 9VOM214; 9VOM414

*(name of object to be tested, type, model, quantity,  
type – portable, fixed, for walling in and other)*

**APPLICANT FOR TEST:** „ELMARK INDUSTRIES“ SC. 2 Dobrudja Blvd. Dobrich, Bulgaria,  
Tel.: 058 500 055, e-mail: [denkov@elmark.bg](mailto:denkov@elmark.bg)

Application Nº 906/ 14.03.2014

*(name of the firm – applicant, address, telephone, number and date of the test application)*

### STANDARD:

- BDS EN 55015:2006+A1:2007+A2:2009 Limits and methods of measurement of radio disturbance characteristics of electrical lighting and similar equipment.  
BDS EN 61000-3-2:2006+A1:2009+A2:2009 Electromagnetic compatibility (EMC).  
Part 3-2: Limits – Limits for harmonic current emissions (equipment input current  $\leq$  16 A per phase).  
BDS EN 61000-3-3:2008 Electromagnetic compatibility (EMC).  
Part 3-3: Limits - Limitation of voltage changes, voltage fluctuations and flicker in public low-voltage supply systems, for equipment with rated current  $\leq$  16 A per phase and not subject to conditional connection.  
BDS EN 61547:2009 Equipment for general lighting purposes - EMC immunity requirements  
BDS EN 61000-4-2:2009 Electromagnetic compatibility (EMC).  
Part 4-2: Testing and measurement techniques - Electrostatic discharge immunity test  
BDS EN 61000-4-4:2004+A1:2010 Electromagnetic compatibility (EMC).  
Part 4-4: Testing and measurement techniques - Electrical fast transient/burst immunity test  
BDS EN 61000-4-5:2006 Electromagnetic compatibility (EMC).  
Part 4-5: Testing and measurement techniques - Surge immunity test  
BDS EN 61000-4-8:2010 Electromagnetic compatibility (EMC).  
Part 4-8: Testing and measurement techniques - Power frequency magnetic field immunity test  
BDS EN 61000-4-11:2004 Electromagnetic compatibility (EMC).  
Part 4-11: Testing and measurement techniques–Voltage dips, short interruptions and voltage variations immunity tests  
*(number and name of the standards)*

**DATE OF ACCEPTANCE IN THE TEST LABORATORY:** 21.03.2014

**YEAR OF PRODUCTION :** 2014  
*(identification number)*

**MANUFACTURER:** „ELMARK INDUSTRIES“ SC. 2 Dobrudja Blvd. Dobrich, Bulgaria,  
Tel.: 058 500 055, e-mail: [denkov@elmark.bg](mailto:denkov@elmark.bg)  
*(firm, trade mark, address)*

**DECLARED TECHNICAL DATA:** Rated voltage – 230 V AC  
Rated frequency – 50 Hz  
Rated power – 4x14 W  
Class I

**DATE OF TEST PERFORMANCE:** 30.05.2014 - 17.06.2014

**LABORATORY CHIEF:** .....

/ T. Hristov /





**I. Emission of Radio disturbance characteristics of electrical lighting and similar equipment**


**1. Radiated electromagnetic disturbances – 9kHz ÷ 30MHz**

BDS EN 55015, cl. 4.4 – Radiated electromagnetic disturbances, limits – Table 3  
 BDS EN 55015, cl. 5.2.4 – Other luminaires  
 BDS EN 55015, cl. 6 – Operating conditions for lighting equipment  
 BDS EN 55015, cl. 6.4 – Ambient temperature: 24 °C ; Relative Humidity: 44 %.  
 BDS EN 55015, cl.9.1 – Measuring arrangement and procedure  
 BDS EN 55015, cl.9.2 – Indoor and outdoor luminaires  
 The test is performed at supply voltage: 230 V

**RESULTS OF MEASUREMENT :**

Frequency	Radiated electromagnetic disturbances - measured along the axis - X		
	Quasi peak - QP		
	Measuring	Margin	Limit
MHz	dB(μA)	dB(μA)	dB(μA)
0,036	28,86	59,14	88,00
0,037	20,19	67,81	88,00
0,108	5,36	65,49	70,85
0,205	6,51	47,73	54,24
0,280	-3,27	53,76	50,49
0,305	2,11	47,36	49,47
0,405	0,31	45,75	46,06
0,455	3,41	41,25	44,66
0,935	-12,15	48,15	36,00
1,495	7,25	23,11	30,36
1,585	10,22	19,44	29,66
2,125	6,26	19,88	26,14
2,950	0,27	21,93	22,20
3,000	-1,01	23,01	22,00
4,745	-16,05	38,05	22,00
20,015	-18,26	40,26	22,00

Drawing of Radiated electromagnetic disturbances - measured along the axis - X

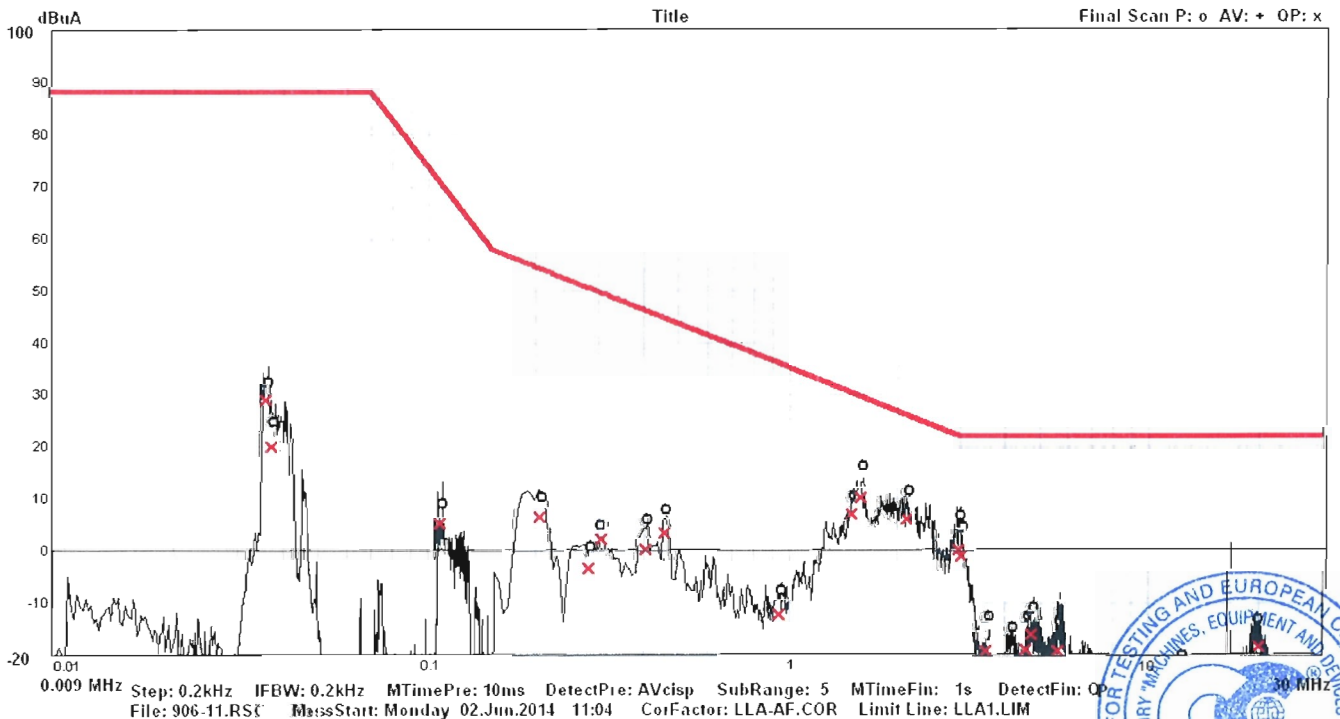


*The results showed in present test report concern tested sample only  
 The test report could be reproduced as a whole only and after written permission of the laboratory*





Frequency MHz	Radiated electromagnetic disturbances - measured along the axis - Y		
	Quasi peak - QP		
	Measuring dB(μA)	Margin dB(μA)	Measuring dB(μA)
0,036	33,88	54,12	88,00
0,041	18,16	69,84	88,00
0,107	9,30	62,14	71,44
0,205	9,33	44,91	54,24
0,250	2,79	49,07	51,86
0,290	-1,09	51,16	50,07
0,405	-6,06	52,12	46,06
0,490	-9,79	53,56	43,77
0,965	-9,68	45,31	35,63
1,470	5,26	25,31	30,57
1,590	9,12	20,50	29,62
2,150	1,56	24,44	26,00
2,860	-5,09	27,66	22,57
3,000	-8,07	30,07	22,00
4,125	-22,64	44,64	22,00
4,200	-22,14	44,14	22,00

Drawing of Radiated electromagnetic disturbances - measured along the axis - Y

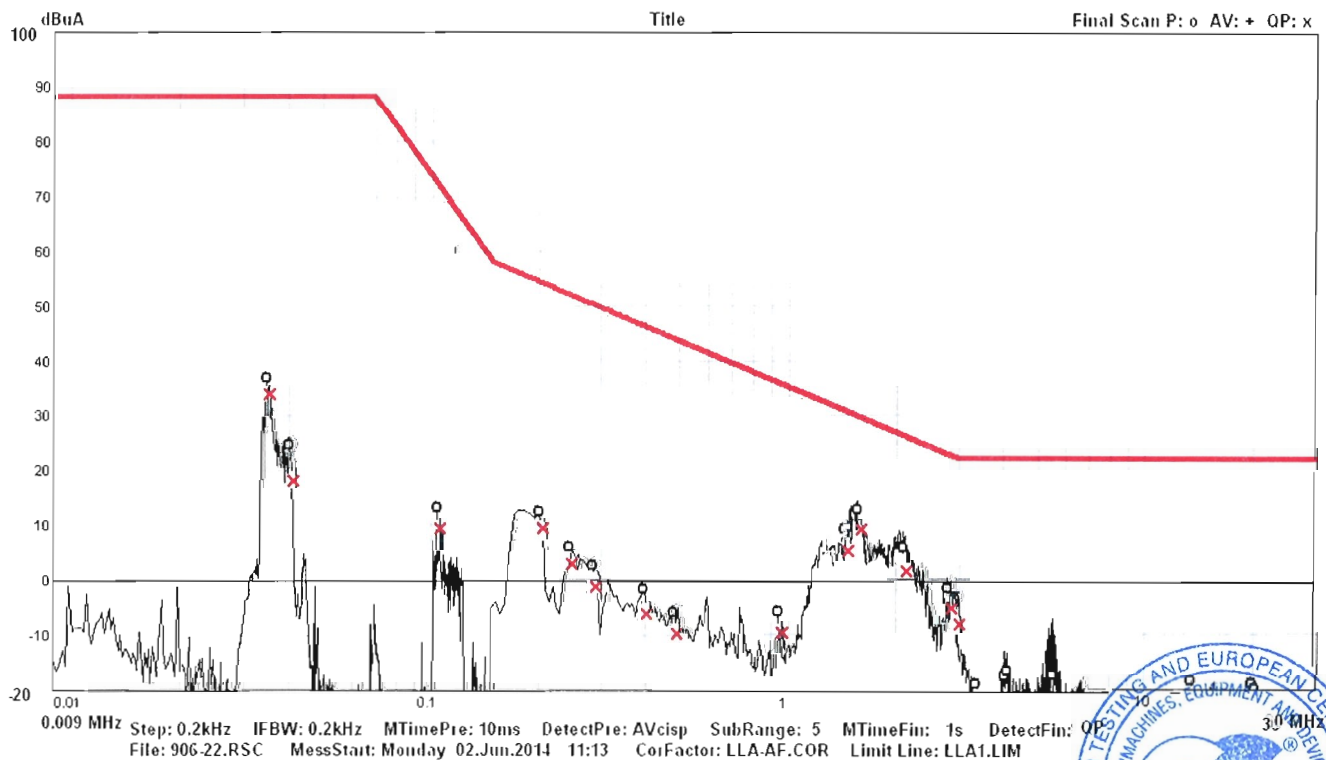


The results showed in present test report concern tested sample only  
The test report could be reproduced as a whole only and after written permission of the laboratory





Frequency	Radiated electromagnetic disturbances - measured along the axis - Z		
	Quasi peak - QP		
	Measuring	Margin	Measuring
MHz	dB(μA)	dB(μA)	dB(μA)
0,036	20,16	67,84	88,00
0,195	-3,41	58,25	54,84
0,285	-11,58	61,86	50,28
0,305	0,32	49,15	49,47
0,390	-2,60	49,11	46,51
0,455	-1,40	46,06	44,66
0,610	-6,43	47,57	41,14
1,490	-10,47	40,87	30,40
1,615	-5,85	35,29	29,44
2,110	-7,51	33,73	26,22
2,890	-12,68	35,12	22,44
3,000	-21,70	43,70	22,00
3,420	-25,18	47,18	22,00
4,495	-23,55	45,55	22,00
4,630	-27,83	49,83	22,00
30,000	-22,22	44,22	22,00

Drawing of Radiated electromagnetic disturbances - measured along the axis - Z

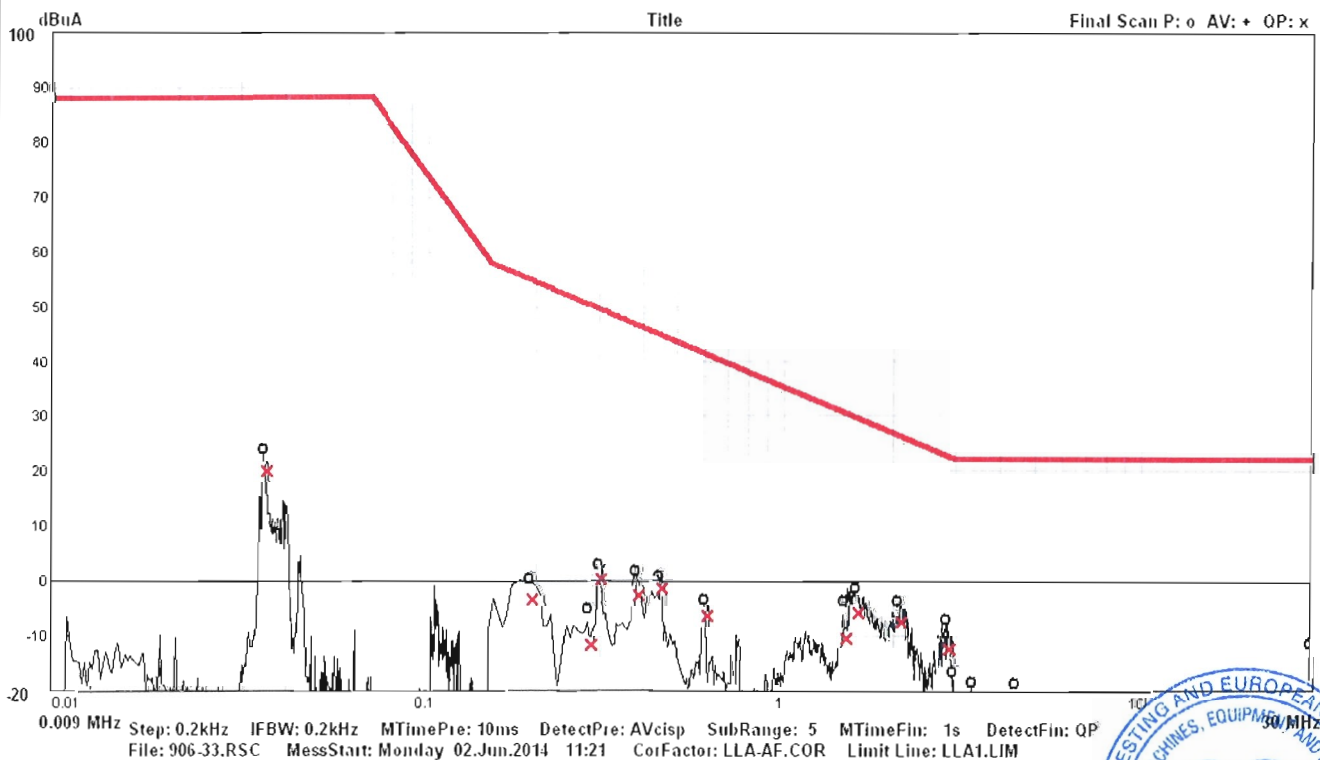

*The results showed in present test report concern tested sample only  
The test report could be reproduced as a whole only and after written permission of the laboratory*




2. Radiated electromagnetic disturbances – 30MHz ÷ 300MHz  
 BDS EN 55015, cl. 4.4.2 – Frequency range 30MHz to 300MHz – Annex B. Limits - Table B.1  
 BDS EN 55015, cl. 5.2.4 – Other luminaires  
 BDS EN 55015, cl. 6 – Operating conditions for lighting equipment  
 BDS EN 55015, cl. 6.4 – Ambient temperature: 25 °C ; Relative Humidity: 46 %  
 BDS EN 55015, cl.9.2 – Measuring arrangement and procedure related to Subclause 4.4.2

**RESULTS OF MEASUREMENT :**

Frequency	Radiated electromagnetic disturbances		
	Quasi peak - QP		
	Measuring	Margin	Measuring
MHz	dB(μV)	dB(μV)	dB(μV)
49,50	13,07	46,77	59,84
71,60	21,97	34,80	56,77
88,30	45,49	9,54	55,03
135,20	25,34	28,66	54,00
159,70	25,38	28,62	54,00
166,70	14,20	39,80	54,00
200,00	26,11	27,89	54,00
225,50	12,86	41,14	54,00
272,40	20,38	40,62	61,00
294,70	12,17	48,83	61,00

Drawing of Radiated electromagnetic disturbances

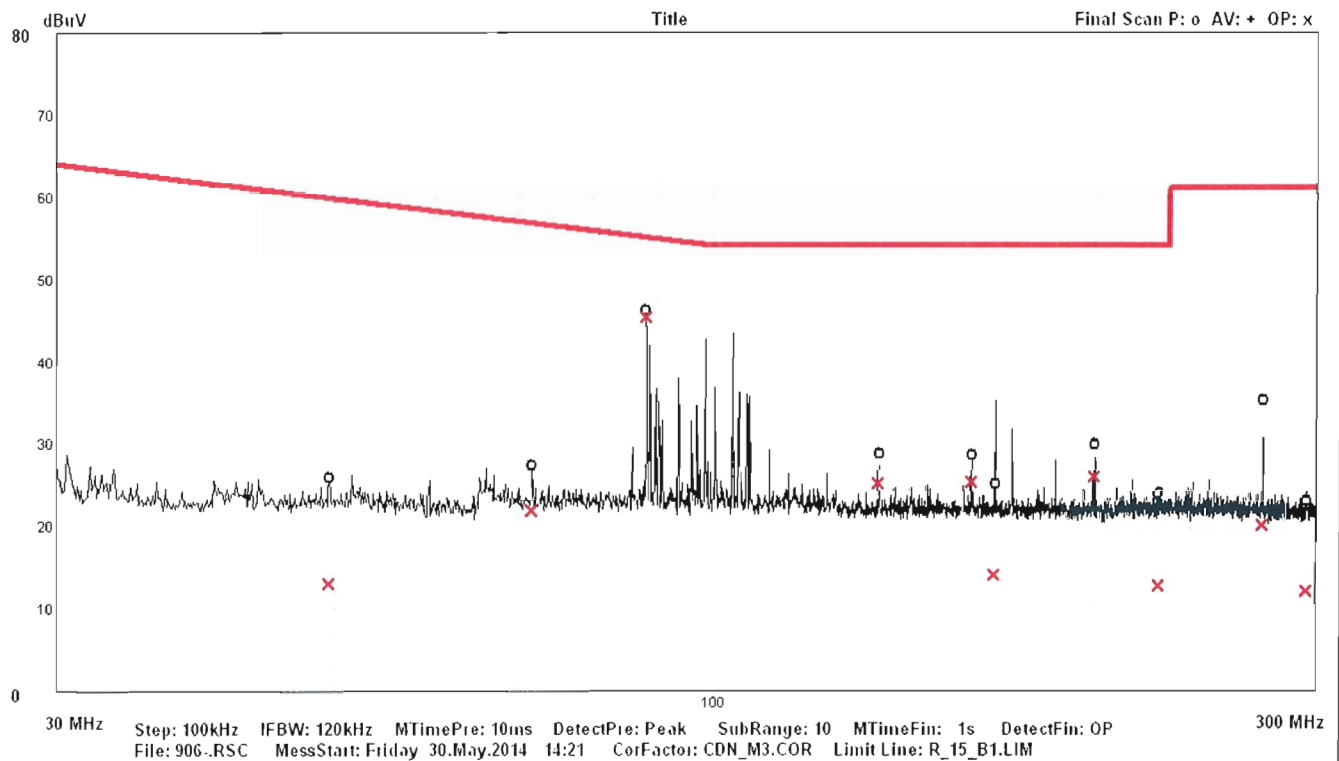

*The results showed in present test report concern tested sample only  
 The test report could be reproduced as a whole only and after written permission of the laboratory*





### 3. HARMONIC CURRENT MEASUREMENT

Classification of equipment - C

Duration of test - 2,5 min

THC= 0,0511 A

I-THD= 19,356 %

POHC= 0,007096 A

POHC Limit= 0,025112 A

$V_{RMS}$  = 229,6 V

$I_{peak}$  = 0,4363 A

Frequency = 50 Hz

$I_{RMS}$  = 0,2698 A

$I_F$  = 0,2647 A

Power = 60,1 W

Crest Factor = 1,617

Power Factor = 0,97

K Factor = 2,42

Harmonic	AVERAGE VALUES			MAX VALUE		
	Measured	100% Limit	% of Limit	Measured	150% Limit	% of Limit
Nº	, A	, A	%	, A	, A	%
2	0,0005	0,0053	9	0,0005	0,0080	7
3	0,0458	0,0770	59	0,0463	0,1161	40
5	0,0064	0,0265	24	0,0067	0,0399	17
7	0,0144	0,0185	78	0,0148	0,0279	53
9	0,0093	0,0132	70	0,0095	0,0200	48
11	0,0071	0,0079	90	0,0075	0,0120	63
13	0,0042	0,0079	53	0,0045	0,0120	37
15	0,0057	0,0079	72	0,0060	0,0120	51
17	0,0040	0,0079	50	0,0043	0,0120	36
19	0,0035	0,0079	45	0,0039	0,0120	32
21	0,0026	0,0079	33	0,0029	0,0120	24
23	0,0031	0,0079	39	0,0034	0,0120	28
25	0,0025	0,0079	32	0,0028	0,0120	23
27	0,0025	0,0079	32	0,0028	0,0120	23
29	0,0017	0,0079	21	0,0019	0,0120	16
31	0,0028	0,0079	36	0,0031	0,0120	26
33	0,0012	0,0079	15	0,0014	0,0120	12
35	0,0017	0,0079	22	0,0019	0,0120	16
37	0,0010	0,0079	12	0,0012	0,0120	10
39	0,0022	0,0079	28	0,0024	0,0120	

The results showed in present test report concern tested sample only  
The test report could be reproduced as a whole only and after written permission of the laboratory





Harmonics of power supply source


$V_{RMS} = 229,6 \text{ V}$	$I_{peak} = 0,4363 \text{ A}$	Frequency = 50 Hz
$I_{RMS} = 0,2698 \text{ A}$	$I_f = 0,2647 \text{ A}$	Power = 60,1 W
	Power Factor = 0,97	

Harmonic	Measured	100% Limit	% of Limit
№	V	V	%
2	0,1385	0,459	30,2
3	0,4098	2,066	19,8
4	0,3041	0,459	66,2
5	0,6257	0,918	68,1
6	0,1837	0,459	40,0
7	0,1168	0,689	17,0
8	0,1607	0,459	35,0
9	0,3444	0,459	75,0
10	0,1378	0,459	30,0
11	0,1148	0,230	50,0
12	0,1148	0,230	50,0
13	0,1148	0,230	50,0
14	0,0918	0,230	40,0
15	0,0462	0,230	20,1
16	0,0918	0,230	40,0
17	0,1110	0,230	48,3
18	0,0689	0,230	30,0
19	0,0903	0,230	39,3
20	0,0689	0,230	30,0
21	0,0459	0,230	20,0
22	0,1137	0,230	49,5
23	0,0856	0,230	37,3
24	0,0689	0,230	30,0
25	0,1215	0,230	52,9
26	0,0689	0,230	30,0
27	0,0375	0,230	16,3
28	0,0689	0,230	30,0
29	0,0459	0,230	20,0
30	0,0689	0,230	30,0
31	0,2196	0,230	95,6
32	0,0658	0,230	28,7
33	0,0230	0,230	10,0
34	0,0689	0,230	30,0
35	0,0346	0,230	15,1
36	0,0689	0,230	30,0
37	0,0230	0,230	10,0
38	0,0918	0,230	40,0
39	0,1972	0,230	85,9
40	0,0935	0,230	40,7


The results showed in present test report concern tested sample only  
The test report could be reproduced as a whole only and after written permission of the laboratory



Current and voltage waveform

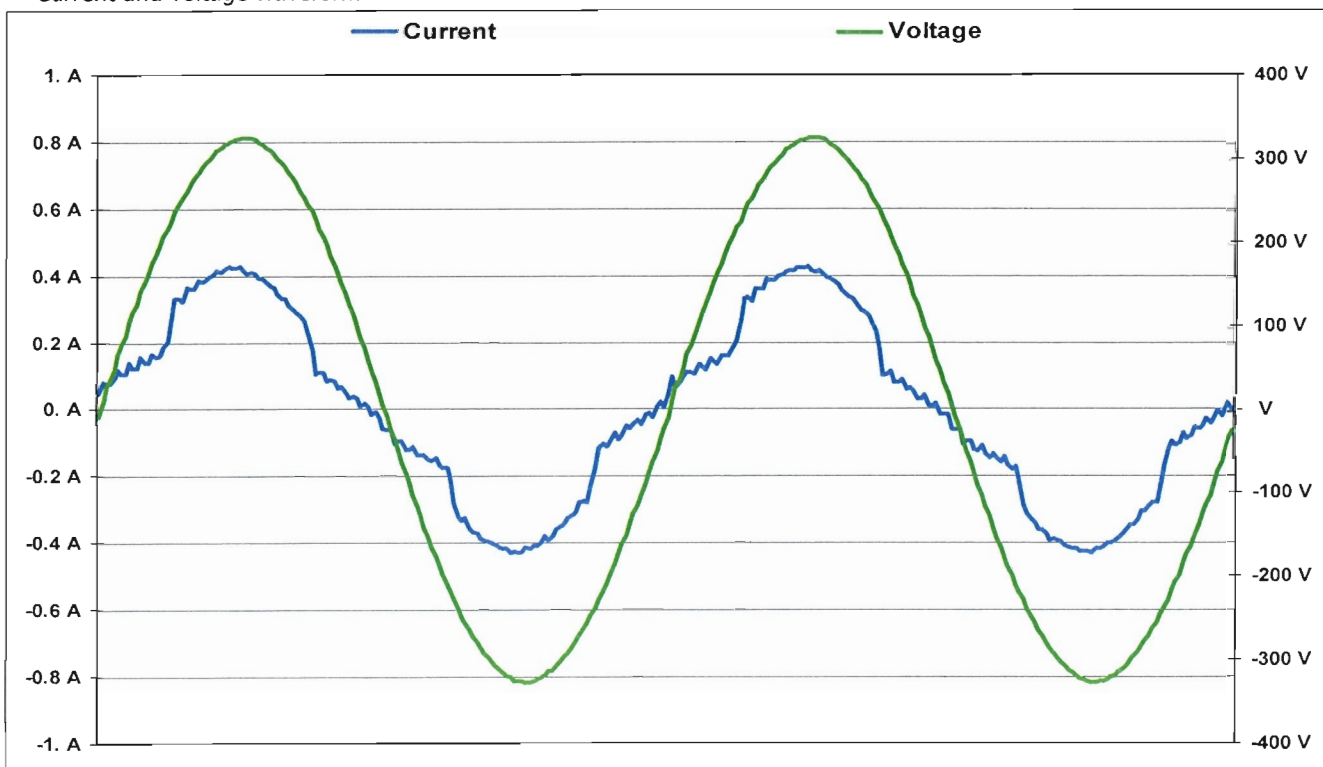

Graphics harmonics

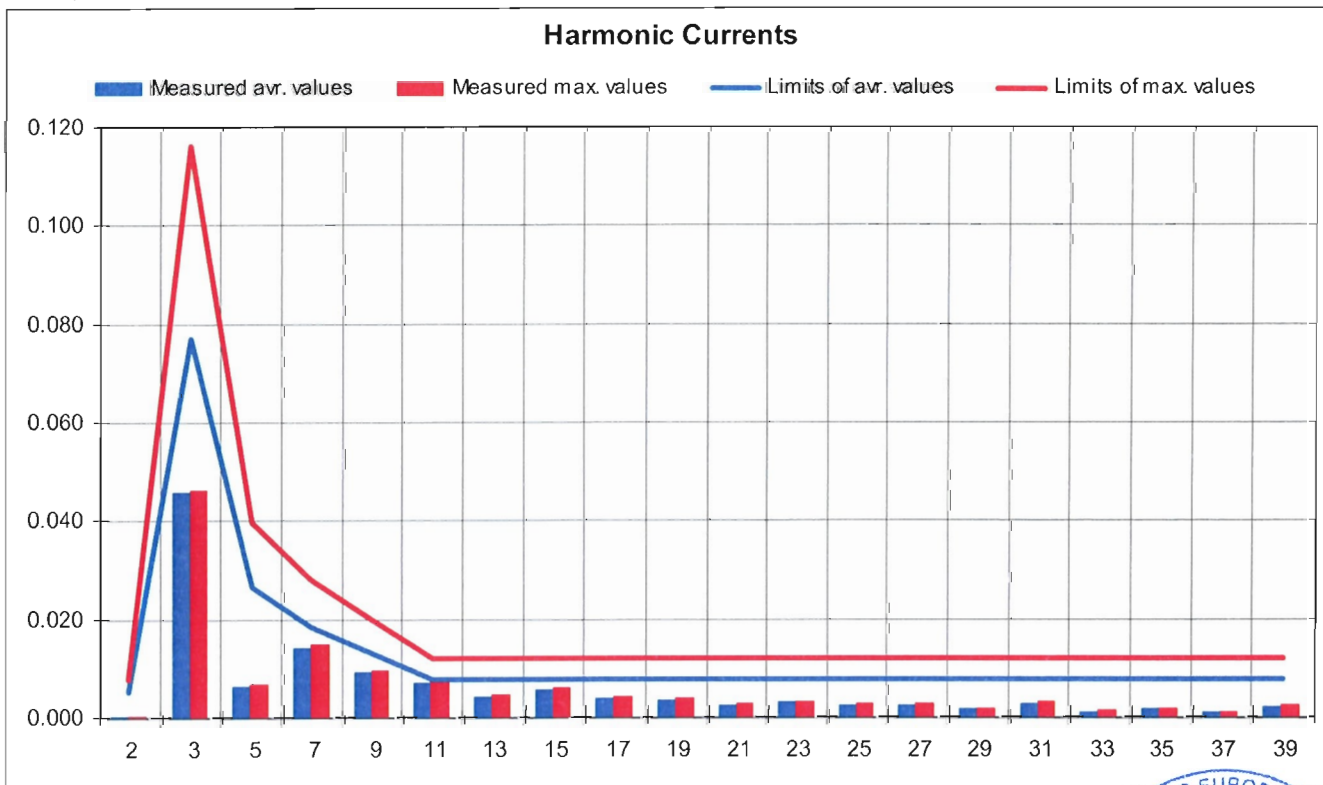

*The results showed in present test report concern tested sample only  
The test report could be reproduced as a whole only and after written permission of the laboratory*







#### 4. Voltage fluctuations and flicker measurement

BDS EN 61000-3-3, cl. 4 – Assessment of voltage changes, voltage fluctuations and flicker

BDS EN 61000-3-3, cl. 5 – Limits

BDS EN 61000-3-3, cl. 6 – Test conditions

BDS EN 61000-3-3, cl. 6.5 - Observation period

**According to BDS EN 61000-3-3:2008 – Annex A, clause A.2 luminaire is deemed to satisfy the requirements of the standard without testing of the EUT**



**II. Immunity of Radio disturbance characteristics for general lighting purposes**

**BDS EN 61547 cl. 4.2 – Performance criteria for lighting equipment**

Performance criterion A

During the test, no change of the luminous intensity shall be observed and the regulating control, if any, shall operate during the test as intended.

Performance criterion B

During the test, the luminous intensity may change to any value. After the test, the luminous intensity shall be restored to its initial value within 1 min. Regulating controls need not function during the test, but after the test, the mode of the control shall be the same as before the test provided that during the test no mode changing commands were given.

Performance criterion C

During and after the test, any change of the luminous intensity is allowed and the lamp(s) may be extinguished. After the test, within 30 min, all functions shall return to normal, if necessary by temporary interruption of the mains supply and/or operating the regulating control.

Additional requirement for lighting equipment incorporating a starting device: After the test, the lighting equipment is switched off. After half an hour, it is switched on again. The lighting equipment shall start and operate as intended.

Environment requirements during the test	Ambient temperature	15 to 35 °C
	Relative Humidity	30 to 60 %
	Air pressure	860 to 1060 mbar
Test environment	Ambient temperature	25 °C
	Relative Humidity	42 %
	Air pressure	1010 mbar

*The results showed in present test report concern tested sample only  
The test report could be reproduced as a whole only and after written permission of the laboratory*




**1. IMMUNITY TO ELECTROSTATIC DISCHARGE (ESD)**

BDS EN 61547, т. 5.2 – Electrostatic discharges – Table 1 - Test levels at enclosure port  
 BDS EN 61000-4-2, т. 7 – Test setup  
 BDS EN 61000-4-2, т. 7.2.2 – Table-top equipment , Figure 4  
 BDS EN 61000-4-2, т. 8 – Test procedure

Time interval between discharges	1 s
Discharge impedance	150 pF
Discharge impedance	330 Ω
Performance Criteria according cl.6.3.4 and Table 15 of BDS EN 61547	Criteria B
Number of discharges	10 positive and 10 negative at the selected points

Discharge location	Type of discharge	Level	Test voltage	Polarity	Result
Body of luminaire – <b>X</b>	Contact - Direct	1;2	2;4 kV	+ -	Pass (criteria A)
Vertical coupling plane (VCP) – <b>X</b>	Contact - Direct	1;2	2;4 kV	+ -	Pass (criteria A)
Horizontal coupling plane (HCP) – <b>X</b>	Contact - Direct	1;2	2;4 kV	+ -	Pass (criteria A)

Picture of the object with marked points of discharge locations

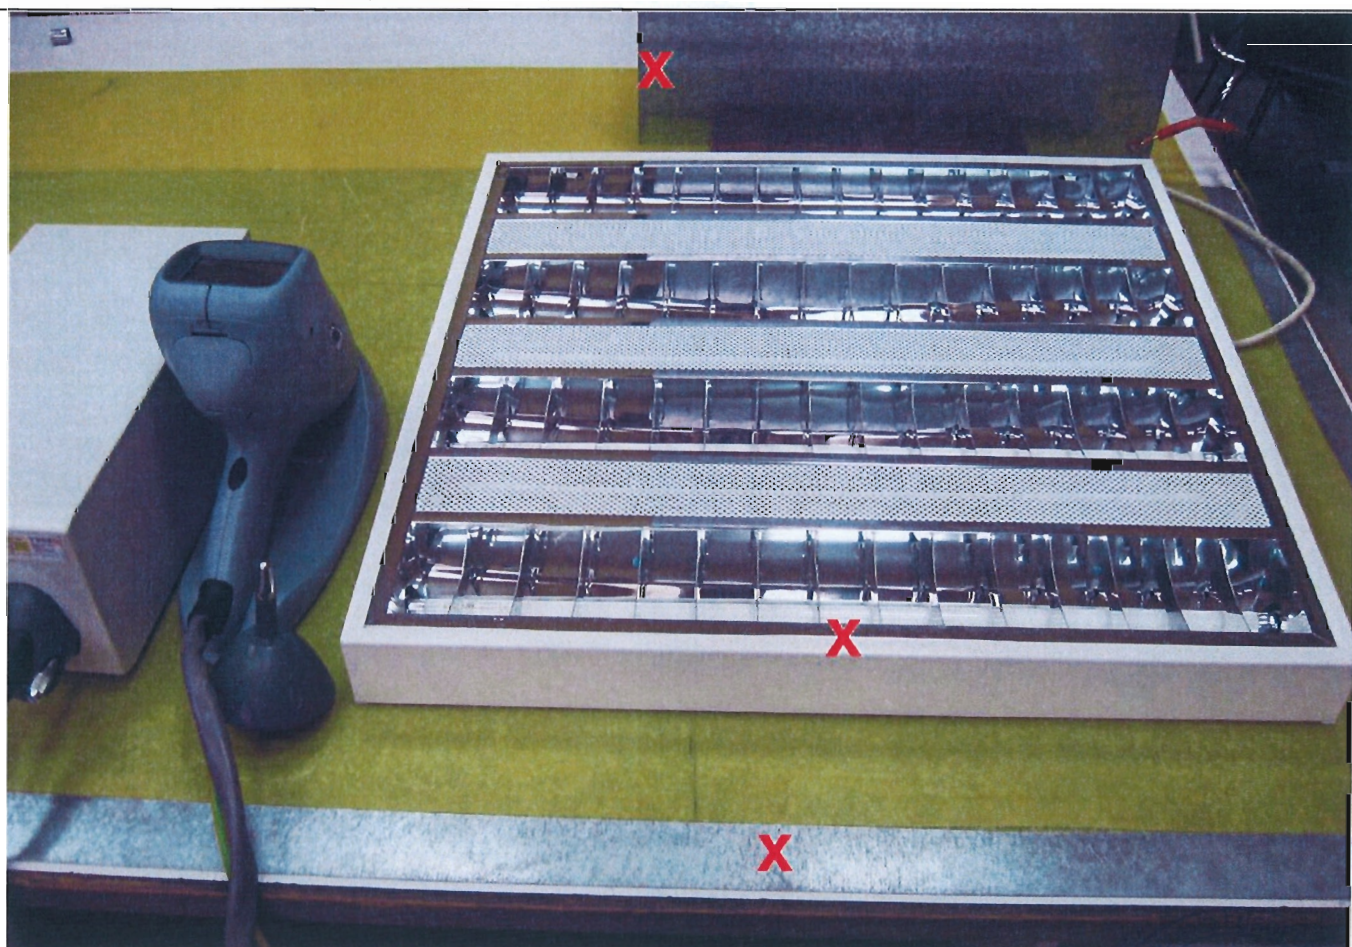

*The results showed in present test report concern tested sample only  
 The test report could be reproduced as a whole only and after written permission of the laboratory*



**2. ELECTRICAL FAST TRANSIENT/BURST IMMUNITY TEST**

BDS EN 61547, т. 5.5 – Applicability ,Table 6

BDS EN 61000-4-4, т. 7 – Test setup

BDS EN 61000-4-4, т. 8 – Test procedure

Rise time	5 ns ±30 %
Duration	50 ns ± 30 %
Repetition frequency	5 kHz
Burst duration	15 ms ± 20 % за 5 kHz
Burst period	300 ms ± 20 %
Time of application	1 min for each polarity and coupling
Performance Criteria according to cl.6.3.4 and Table 15 of BDS EN 61547	Criteria B

Pulse Application	Application	Level	Test Voltage V	Polarity	Result
Between L and Ground plane	Coupling network	1	500	+	Pass (criteria A)
				-	Pass (criteria A)
		2	1000	+	Pass (criteria A)
				-	Pass (criteria A)
Between neutral and Ground plane	Coupling network	1	500	+	Pass (criteria A)
				-	Pass (criteria A)
		2	1000	+	Pass (criteria A)
				-	Pass (criteria A)
Between PE and Ground plane	Coupling network	1	500	+	Pass (criteria A)
				-	Pass (criteria A)
		2	1000	+	Pass (criteria A)
				-	Pass (criteria A)
Between L, neutral, PE and Ground plane	Coupling network	1	500	+	Pass (criteria A)
				-	Pass (criteria A)
		2	1000	+	Pass (criteria A)
				-	Pass (criteria A)

Signal lines

Pulse Application	Application	Level	Test Voltage V	Polarity	Result
-	Coupling clamp	1	500	+	-
				-	-
-	Coupling clamp	2	1000	+	-
				-	-

Control lines

Pulse Application	Application	Level	Test Voltage V	Polarity	Result
-	Coupling clamp	1	500	+	-
				-	-
-	Coupling clamp	2	1000	+	-
				-	-

*The results showed in present test report concern tested sample only  
The test report could be reproduced as a whole only and after written permission of the laboratory*





**3. SURGE IMMUNITY TEST**

BDS EN 61547, τ. 5.7 – Applicability ,Table 10  
BDS EN 61000-4-5, τ. 7 – Test setup  
BDS EN 61000-4-2, τ. 8 – Test procedure

Front time	1,2 μs ± 30 %	
Time to half value	50 μs ± 20 %	
Source impedance	Power line symmetrical Power line unsymmetrical	2 Ω + 18 μF 12 Ω + 9 μF
Phase angles	90°/ 270°	
Number of surges / polarity /phase angle	5	
Performance Criteria according to cl.6.3.4 and Table 15 of BDS EN 61547	Criteria C	

Power line symmetrical

Pulse Application	Level	Test Voltage V	Polarity	Result
phase L – neutral N	1	500	+	Pass (criteria A)
			-	Pass (criteria A)
	2	1000	+	Pass (criteria B)
			-	Pass (criteria B)

Power line unsymmetrical

Pulse Application	Level	Test Voltage V	Polarity	Result
phase L – protective earth	1	500	+	Pass (criteria A)
			-	Pass (criteria A)
	2	1000	+	Pass (criteria B)
			-	Pass (criteria B)
	3	2000	+	Pass (criteria B)
			-	Pass (criteria B)
neutral N - protective earth	1	500	+	Pass (criteria A)
			-	Pass (criteria A)
	2	1000	+	Pass (criteria B)
			-	Pass (criteria B)
	3	2000	+	Pass (criteria B)
			-	Pass (criteria B)

*The results showed in present test report concern tested sample only  
The test report could be reproduced as a whole only and after written permission of the laboratory*





#### 4. RATED POWER FREQUENCY MAGNETIC FIELD

BDS EN 61547, τ. 5.4 – Applicability ,Table 3

BDS EN 61000-4-8 τ. 7 – Test setup

BDS EN 61000-4-8 τ. 8 – Test procedure

Performance Criteria according to cl.6.3.3  
and Table 15 of BDS EN 61547

Criteria A

Standard inductive coil	Orientation of standard inductive coil	Level	Field strength in the centre for all other inductive coils	Current in the coil (a coil with 10 windings)	Result
1 m x 1 m	X	2	3 A/m	3,45 A	Pass (criteria A)
1 m x 1 m	Y	2	3 A/m	3,45 A	Pass (criteria A)
1 m x 1 m	Z	2	3 A/m	3,45 A	Pass (criteria A)

*The results showed in present test report concern tested sample only  
The test report could be reproduced as a whole only and after written permission of the laboratory*





## 5. Voltage dips, short interruptions and voltage variations immunity tests

### 5.1 Voltage dips immunity tests

BDS EN 61547, τ. 5.8 – Applicability ,Table 11

BDS EN 61000-4-11 τ. 7 – Test setup

BDS EN 61000-4-11 τ. 8 – Test procedure

BDS EN 61000-4-11 τ. 8.2.1 – Testing for each selected combination of test level and duration with a sequence of three dips with intervals of 10 s minimum (between each test event)

Performance Criteria according to cl.6.3.4 and Table 15 of BDS EN 61547

Criteria C

Voltage test levels ( % of rated voltage)	Duration (cycles)	Phase angle synchronization	Result
70 %	10 cycles	0°	Pass (criteria B)

### 5.2 Short interruptions immunity tests

BDS EN 61547, τ. 5.8 – Applicability ,Table 12

BDS EN 61000-4-11 τ. 7 – Test setup

BDS EN 61000-4-11 τ. 8 – Test procedure

BDS EN 61000-4-11 τ. 8.2.1 – Testing for each selected combination of test level and duration with a sequence of three interruptions with intervals of 10 s minimum (between each test event)

Performance Criteria according to cl.6.3.4 and Table 15 of BDS EN 61547

Criteria B

Voltage test levels ( % of rated voltage)	Duration (cycles)	Phase angle synchronization	Result
0 %	0,5 cycles	0°	Pass (criteria B)





**USED TECHNICAL EQUIPMENTS:**

	<b>Appliance</b>	<b>Type</b>	<b>Manufacturer</b>	<b>Identity №</b>	<b>Last calibration date</b>
1.	ESD - Generator	NSG438	TESEQ Switzerland	988	14.03.2012
2.	EFT/B - Generator	NSG 2050 INA 2050 PNW 2225 CDN 133	Schaffner Electrotest GmbH, Germany	200902-653LU 200906-578LU 200838-570LU 34460	14.03.2012
3.	Surge - Generator	NSG 2050 INA 2050 PNW 2050 CDN 133	Schaffner Electrotest GmbH, Germany	200902-653LU 200906-578LU 200911-636LU 34460	16.03.2012
4.	Digital multimeter	UNIGOR 390	LEM Austria	PI 3288	08.07.2011
5.	Voltage Generator	GL 01-16-230	Neosvet Bulgaria	0001	-
6.	Power Quality Analyzer	435	Fluke Netherlands	DM 9881064	08.11.2011
7.	Thermometer-higrometer	177-H1	TESTO Germany	01320300/902	19.04.2012
8.	EMI – receiver 9 kHz ÷ 1000 MHz	SCR 3501	Schaffner Electrotest GmbH, Germany	522	07.07.2011
9.	Large loop antenna 2m	RF300	Laplace Instruments LTD U.K.	9123	12.03.2013
10.	Coupling/Decoupling network	CDN M2+M3	Frankonia EMC Test - Systems	A2210229	18.04.2013

TEST PERFORMER: 1. ....

/ T. Hristov /



2. ....

/D. Chavalinov /

CHIEF LABORATORY : .....

/ T. Hristov /